

**OPTIC CHARACTERISTICS<sup>1</sup>**

Powers:	+5.0 D to +34.0 D in 0.5 diopter increments									
Model Numbers:	DIU100	DIU150	DIU225	DIU300	DIU375	DIU450	DIU525	DIU600	DIU700	DIU800
Cylinder Powers - IOL Plane	1.00 D	1.50 D	2.25 D	3.00 D	3.75 D	4.50 D	5.25 D	6.00 D	7.00 D	8.00 D
Cylinder Powers - Corneal Plane	0.69 D	1.03 D	1.54 D	2.06 D	2.57 D	3.08 D	3.60 D	4.11 D	4.80 D	5.48 D
Diameter:	6.0 mm									
Shape:	Biconvex, continuous, higher-order aspheric anterior surface									
Material:	UV-light absorbing, hydrophobic acrylic									
Refractive Index:	1.47 at 35° C									
Edge Design:	<b>ProTEC</b> frosted, continuous 360° posterior square edge									


BIOMETRY*	CONTACT ULTRASOUND <sup>†</sup>	OPTICAL <sup>††</sup>
A-Constant:	118.8	119.3
AC Depth:	5.4 mm	5.7 mm
Surgeon Factor: <sup>2</sup>	1.68 mm	1.96 mm

**HAPTIC CHARACTERISTICS<sup>1</sup>**

Overall Diameter:	13.0 mm
Thickness:	0.46 mm
Style:	C, TRI-FIX haptics offset from optic; 1-piece lens
Material:	Soft, Foldable, UV-light absorbing, hydrophobic acrylic
Design:	New squared and frosted haptic design

Preloaded **TECNIS Simplicity®** delivery system

\* Values theoretically derived for a typical 22.0 D lens. Johnson & Johnson Vision recommends that surgeons personalize their A-constant based on their surgical techniques and equipment, experience with the lens model and postoperative results.  
<sup>†</sup> IOL constants have been theoretically derived for contact ultrasound.  
<sup>††</sup> IOL constants have been derived from clinical evaluation results of the 1-Piece IOL Platform.

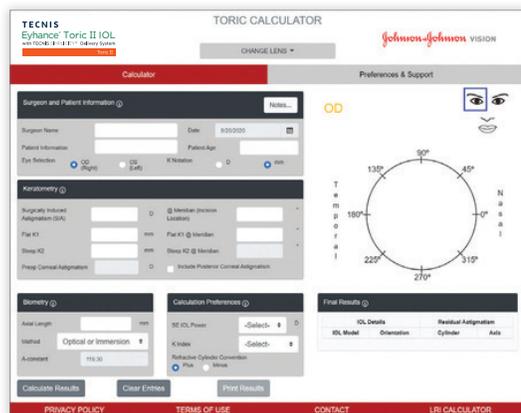

For precise results, utilize the **TECNIS®** Toric Calculator to determine the appropriate Toric model and power. Based on preoperative keratometry, biometry, and surgeon preferences, the calculator provides three IOL options, with residual astigmatism, to assist surgeons in accurate lens model selection and axis placement. [www.TecnisToricCalc.com](http://www.TecnisToricCalc.com)

**References:**

1. **TECNIS Eyhance®** Toric II IOL with **TECNIS Simplicity®** Delivery System, Model DIU - DfU OUS - Z311515P, Rev. A, Sep. 2020. REF2020CT4293.
2. Holladay JT. International Intraocular Lens & Implant Registry 2003. J Cataract Refract Surg. 2003; 29:176-197. REF2016CT0151.

For Healthcare Professionals Only. Please reference the Instructions for Use for a complete list of Indications and Important Safety Information and contact our specialists in case of any questions.